


Selection of TTA Implants

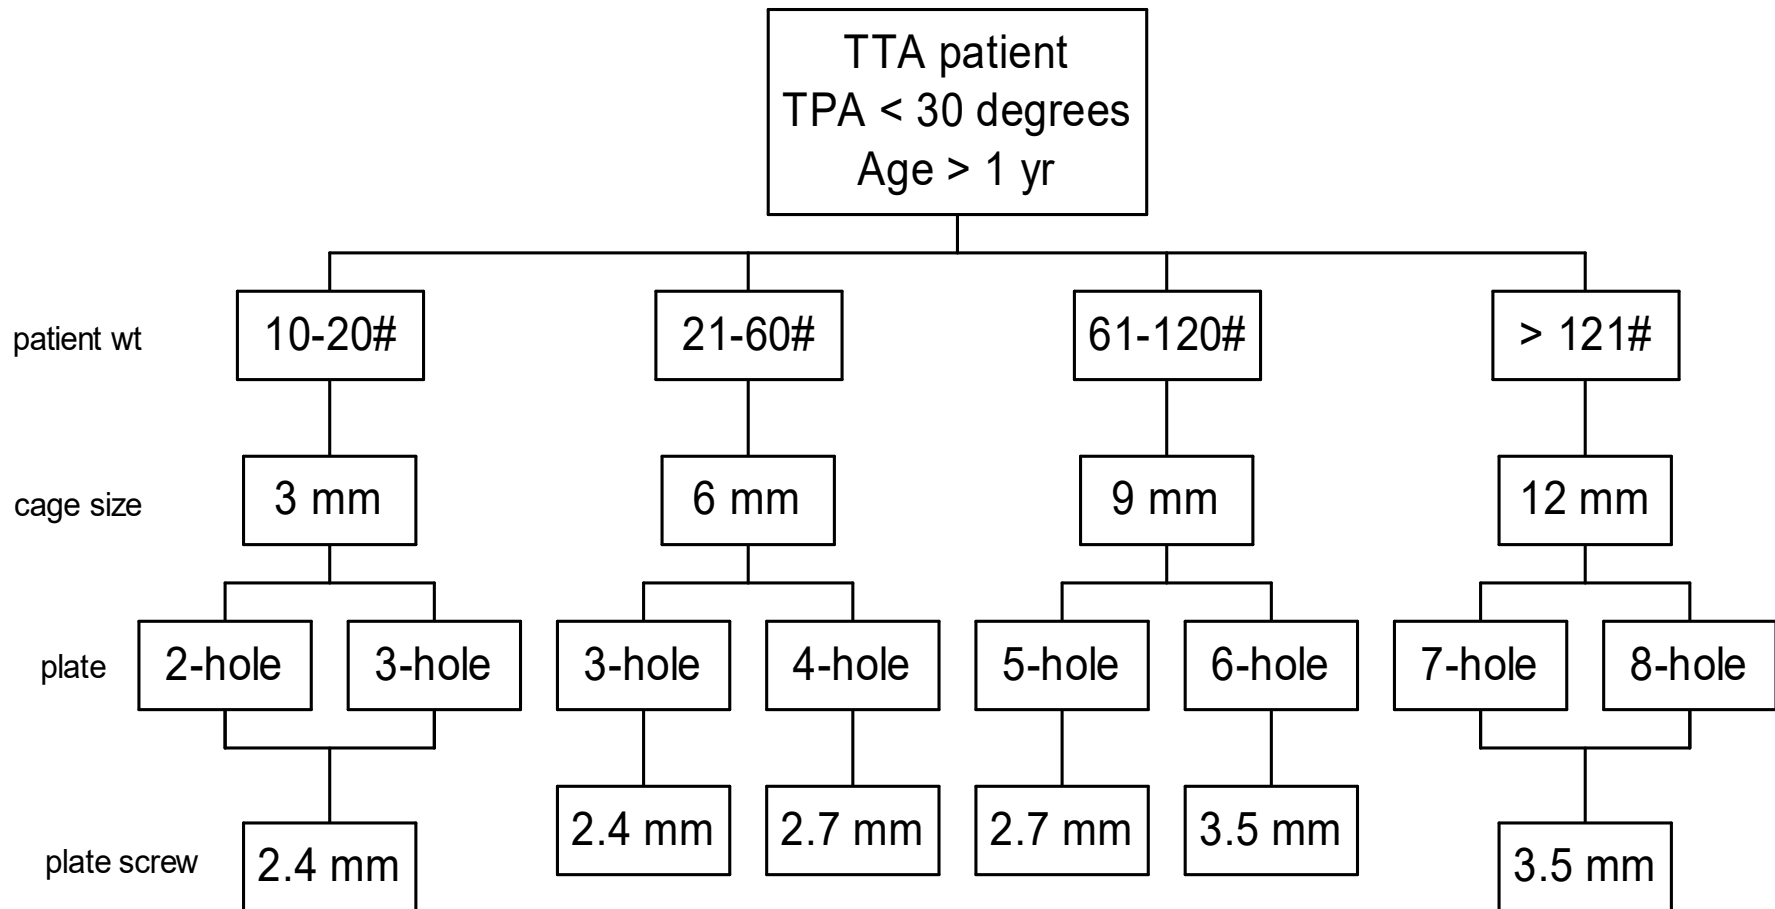

PATIENT WEIGHT: These numbers are estimates; note that there is some overlap between weight ranges given & ½ size cages may be appropriate.
 CAGE SIZE: all cages are secured proximally with 2.4 mm cortical screws; final size should be determined intraoperatively by testing for tibial thrust.
 PLATE: the plate size can be determined from the radiographs preoperatively; final selection may vary in surgery.